



Anderson Instrument Co.
 156 Auriesville Road
 Fultonville, NY 12072
 1-518-922-5315
 Fax 1-800-726-6733
 www.andinst.com

Technical Bulletin

AJ-300 Series Circular Chart Recorder Order Worksheet

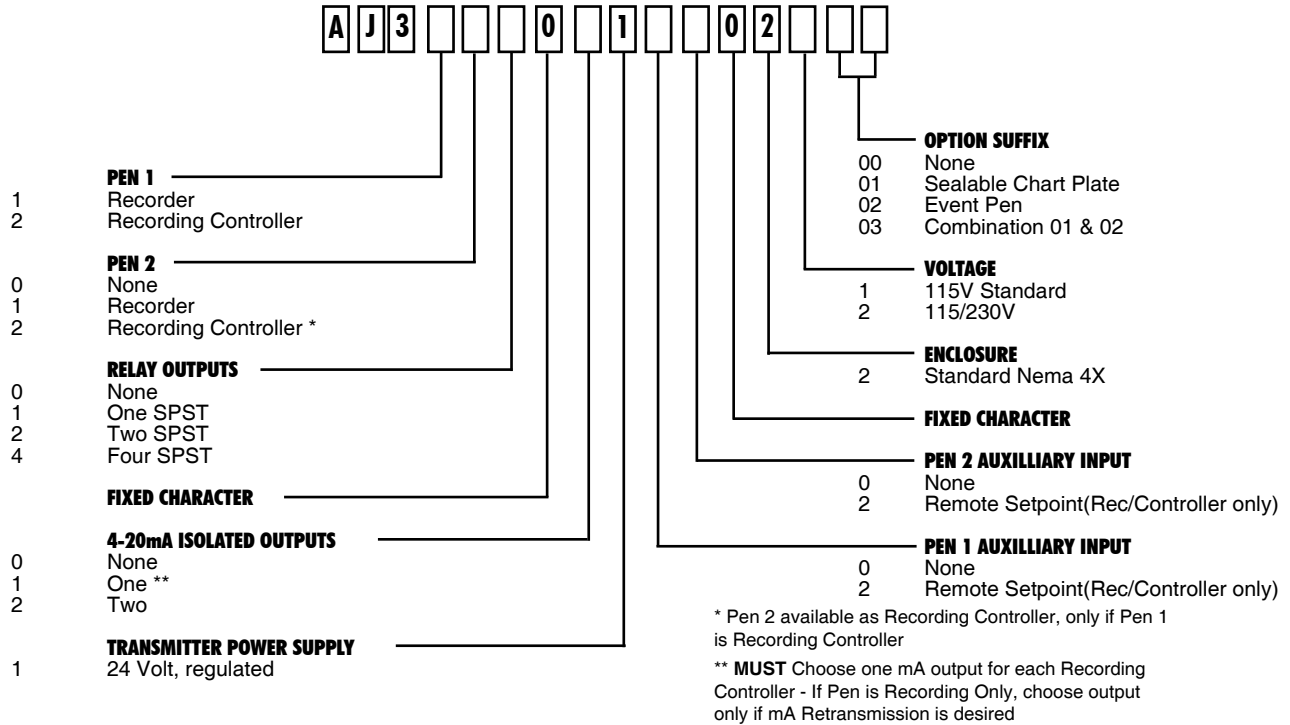


Chart Range - Select One - Consult Factory If Not Listed (Left to Right = Chart Hub to Outer Edge)

00215311 (0-100, 12hr)	00215306 (30-230, 12hr)	00215310 (200-0, 24hr)
00215301 (0-100, 24hr)	00215305 (30-230, 24hr)	00215309 (200-0, 7day)
00215315 (0-150, 24hr)	00215314 (30-230, 7day)	00215302 (230-30, 24hr)
00215303 (0-200, 24hr)	00215308 (50-250, 24hr)	00215312 (100/30-230, 12hr)
00215313 (0-200, 7day)	00215307 (90-190, 12hr)	00215304 (0-100/30-230, 24hr)
00215319 (0-250, 24hr)	00215317 (100-500, 24hr)	00215321 (0-100/110-200, 12hr)
00215316 (0-300, 24hr)	00215318 (200-0, 12hr)	00215320 (0-200/50-250, 24hr)

Pen 1 Color = RED

Note: Relay Outputs, mA Outputs and Controllers require final field setup

Input Type

RTD °F (.00385)
 RTD °C (.00385)
 4-20 mA
 Other _____

Display Range

(Show decimal if required)
 Low: _____
 High: _____
 (May differ from chart range)

Pen 2 Color = GREEN

Note: Relay Outputs, mA Outputs and Controllers require final field setup

Input Type

RTD °F (.00385)
 RTD °C (.00385)
 4-20 mA
 Other _____

Display Range

(Show decimal if required)
 Low: _____
 High: _____
 (May differ from chart range)